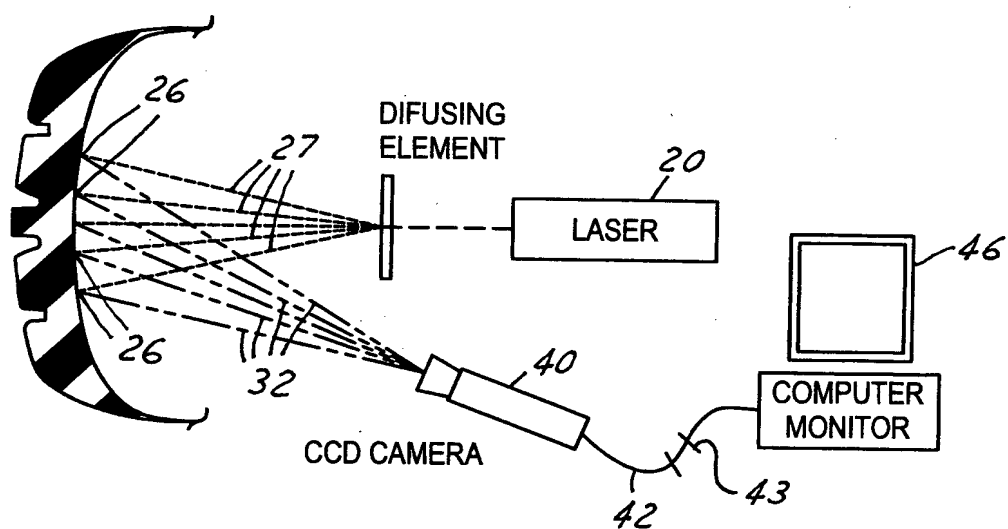
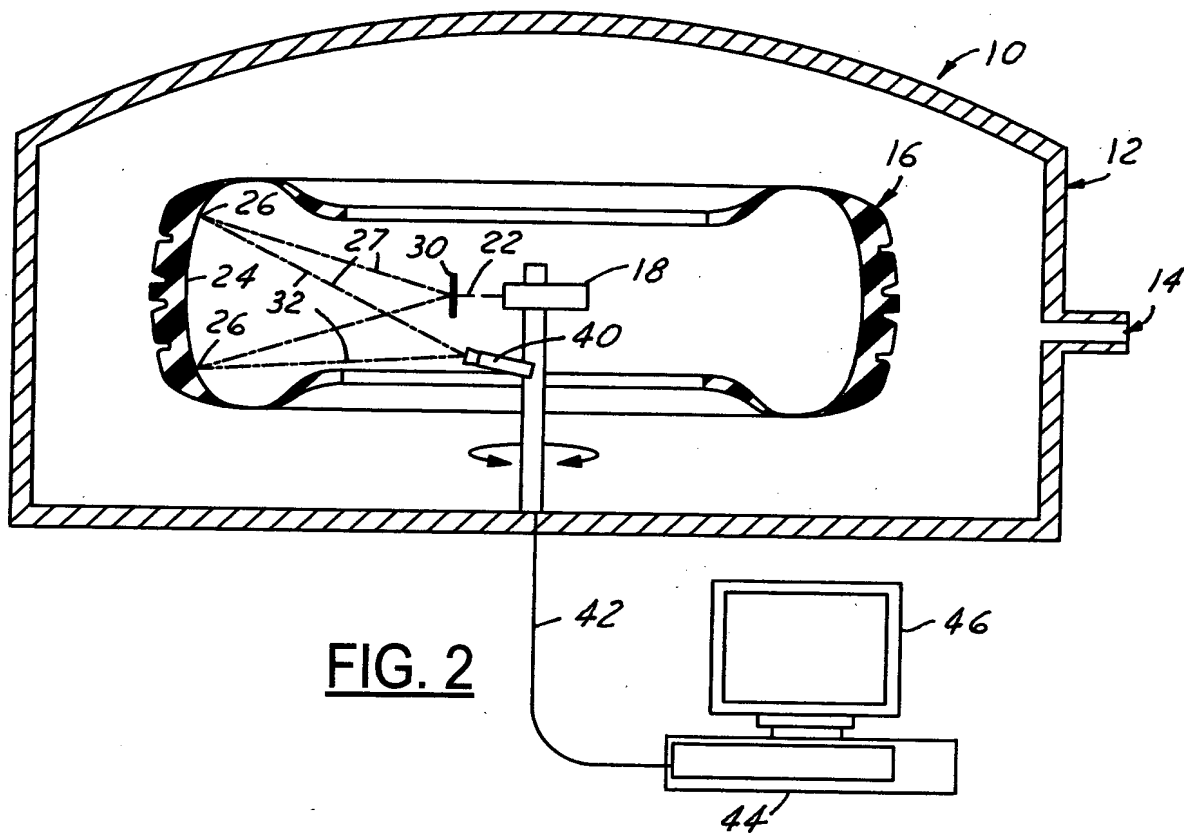
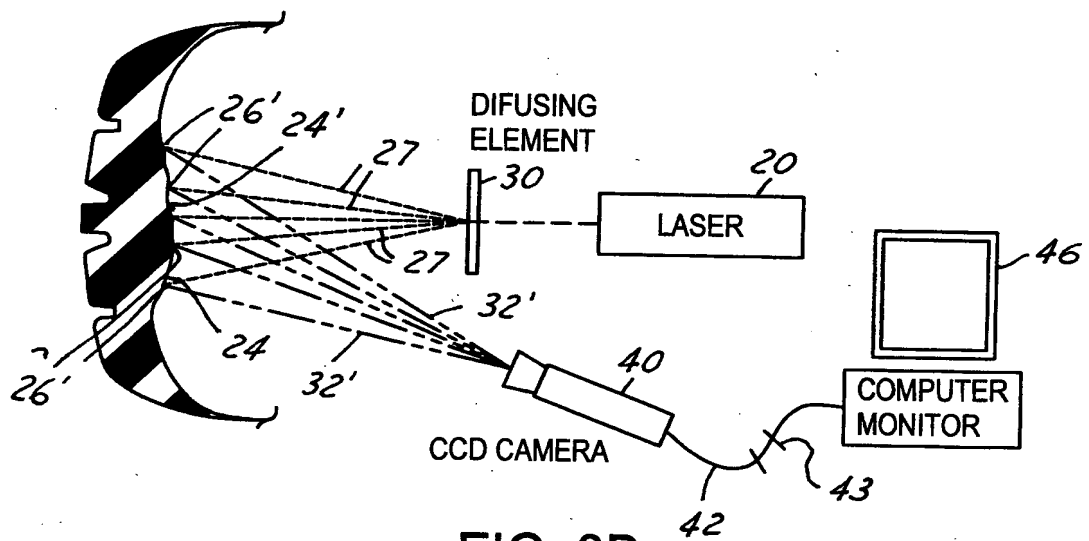


FIG. 1





**FIG. 3B**

Vacuum Level at which Image is Captured (Inches of Hg)	Image Name
0.0	"0_0"
0.5	"0_5"
1.0	"1_0"
1.5	"1_5"
2.0	"2_0"
2.5	"2_5"

FIG. 4A

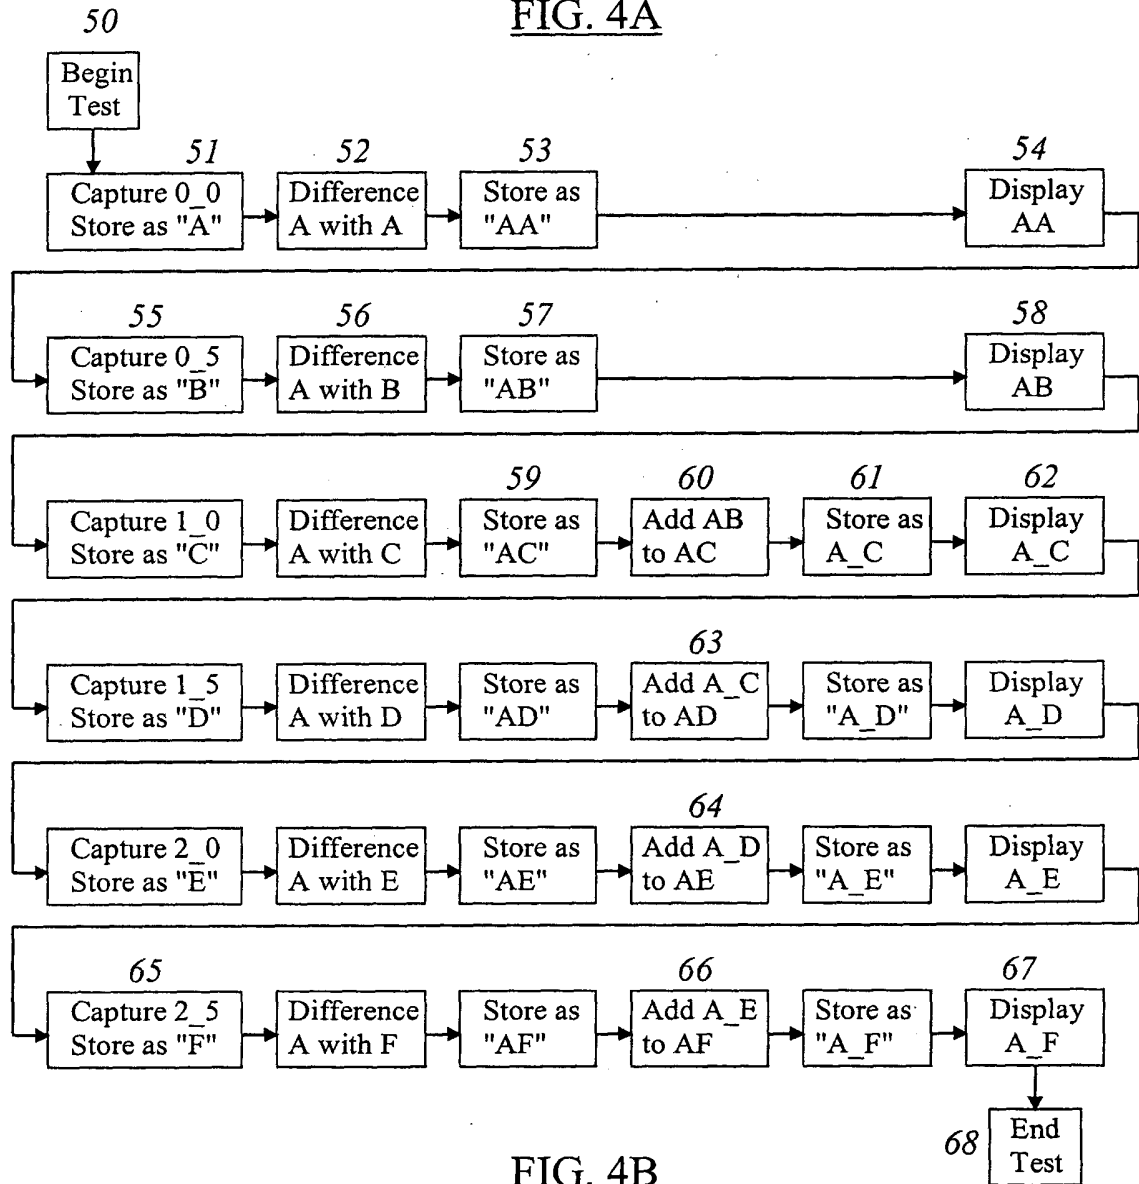


FIG. 4B

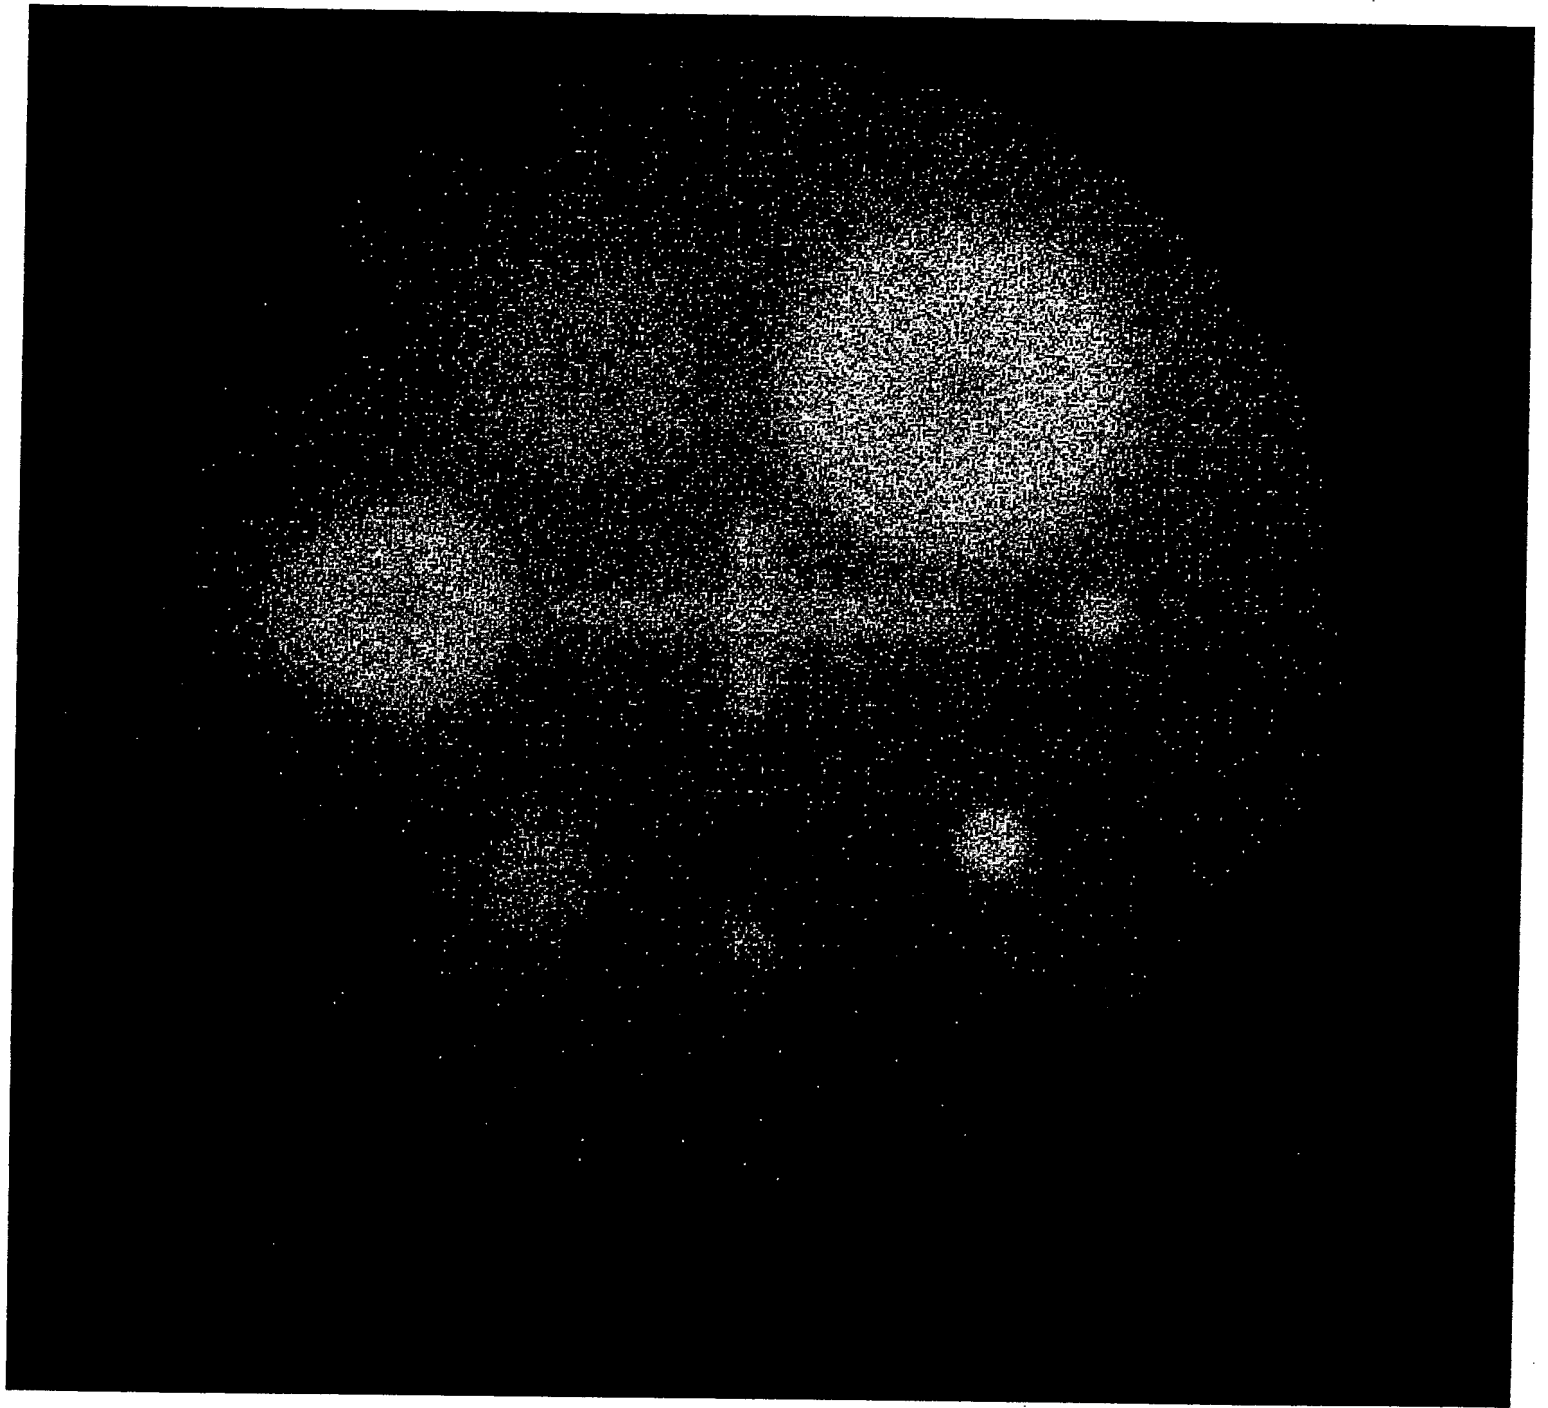


FIGURE 5